


GLOBAL REPORT

No of participants: 75

No of responded participants: 72


Response percentage: 96 %

Summary




Summary	AVR success rate
Sample S001	99.3 %
Sample S002	95.7 %
Average:	97.5 %

Sample S001




Sample S001 results	Responded	AVR success rate	Count
	Clinical interpretation	100 %	83
	BorrAb	100 %	6
	BorrAbG	98.8 %	81
	BorrAbM	98.6 %	72
Total:		99.3 %	242

Sample S001 Clinical interpretation

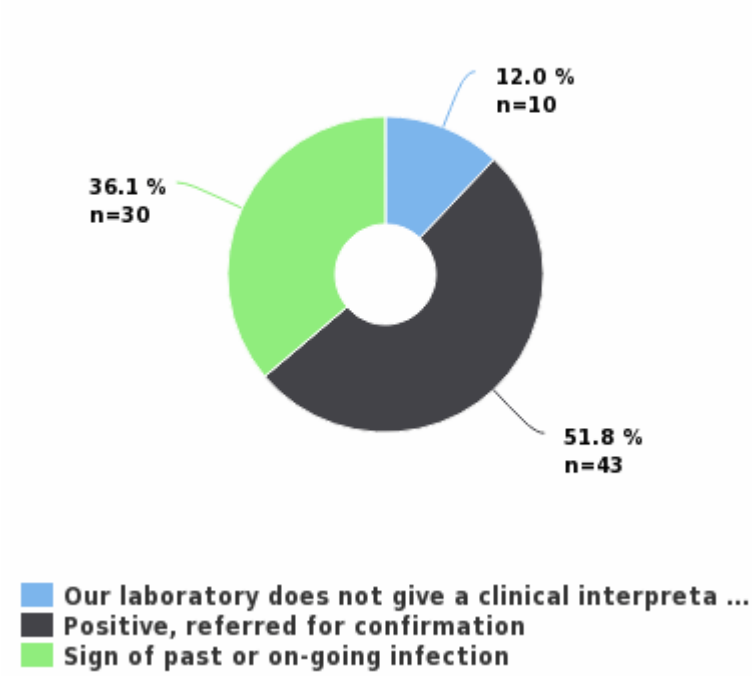


Clinical interpretation	Interpretation	Additional information	Interpretation count	Additional information count	AVR success rate	Interpretation score
	Sign of past or on-going infection		30		100 %	4
	Positive, referred for confirmation		43		100 %	4
	Our laboratory does not give a clinical interpretation to the physician		10		-	-
	Total:		83		100 %	


Sample S001 BorrAb



Sample S001 BorrAbG



Sample S001 BorrAbM



BorrAb	Interpretation	Method	Interpretation count	Method count	AVR success rate	Interpretation score
	Positive		6		100 %	2
		Immunetics C6-LYME-ELISA		6		
	Total:		6		100 %	


BorrAbG	Interpretation	Method	Interpretation count	Method count	AVR success rate	Interpretation score
	Negative		1		0 %	0
		Thermo Scientific IDEIA Borrelia Burgdorferi IgG		1		
	Positive		80		100 %	2
		Aesku Diagn AESKULISA Borrelia IgG ELISA		1		
		Biomedica Borrelia IgG ELISA		1		
		bioMérieux VIDAS Lyme IgG		20		
		Diasorin LIAISON Borrelia IgG		28		
		Euroimmun Anti-Borrelia plus VlsE Elisa IgG		1		
		Euroimmun Anti-Borrelia Select ELISA IgG		1		
		Euroimmun Westernblot/ EUROLINE-WB IgG		2		
		In-house IFA		1		
		In-house Borrelia IgG ELISA		1		
		Medac Borrelia-IgG-Elisa		1		
		Mikrogen ELISA Recomwell IgG/IgM		1		
		Mikrogen Line Blot Recomblot IgG		4		
		Mikrogen recomBead Borrelia IgG		1		
		Mikrogen recomLine Borrelia IgG		2		
		Orgentec Borrelia IgG Recomb.		3		
		Siemens Enzygnost Borreliosis IgG		7		
		Viramed Borrelia ViraStripe IgG		1		
		Vircell VirClia Borrelia IgG		1		
		Virion/Serion Borrelia burgdorferi IgG ELISA		1		
		Virotech Borrelia afzelii + VlsE IgG Europe ELISA		1		
		Virotech Borrelia Europe plus TpN17 LINE IgG		1		
	Total:		81		98.8 %	

BorrAbM	Interpretation	Method	Interpretation count	Method count	AVR success rate	Interpretation score
	Negative		1		0 %	0
		Thermo Scientific IDEIA Borrelia Burgdorferi IgM		1		
	Borderline		3		100 %	2
		Diasorin LIAISON Borrelia IgM		1		
		In-house IFA		1		
		In-house Borrelia IgM ELISA		1		
	Positive		68		100 %	2
		Aesku Diagn AESKULISA Borrelia IgM ELISA		1		
		Biomedica Borrelia IgM ELISA		1		
		bioMérieux VIDAS Lyme IgM		17		
		Diasorin LIAISON Borrelia IgM		23		
		Euroimmun Anti-Borrelia Select ELISA IgM		1		

Copyright © Labquality Oy  
Labquality does not permit any reproduction for commercial purposes of any portion of the material subject to this copyright. Labquality prohibits any use of its name, or reference to Labquality EQA program, or material in this report in any advertising, brochures or other commercial publications. Labquality EQA data do not necessarily indicate the superiority of instruments, reagents, testing equipments or materials used by participating laboratories. Use of Labquality EQA data to suggest superiority or inferiority of equipments or materials may be deceptive and misleading. Proficiency test results are handled confidentially. Labquality will not issue any statements to third parties of the performance of laboratories in external quality assessment schemes unless otherwise agreed.


		Euroimmun Lyme screen ELISA IgM		1		
		Euroimmun Westernblot/ EUROLINE-WB IgM		2		
		Medac Borrelia-IgM-Elisa		1		
		Mikrogen Line Blot Recomblot IgM		3		
		Mikrogen recomBead Borrelia IgM		1		
		Mikrogen recomLine Borrelia IgM		3		
		Orgentec Borrelia IgM Recomb.		2		
		Siemens Enzygnost Borreliosis IgM		7		
		Viramed Borrelia ViraStripe IgM		1		
		Vircell VirClia Borrelia IgM		1		
		Virion/Serion Borrelia burgdorferi IgM ELISA		1		
		Virotech Borrelia afzelii IgM ELISA		1		
		Virotech Borrelia Europe LINE IgM Line Immunoblot		1		
	Total:		72		98.6 %	

Sample S002




Sample S002 results	Responded	AVR success rate	Count
	Clinical interpretation	98.6 %	83
	BorrAb	100 %	6
	BorrAbG	98.8 %	81
	BorrAbM	86.1 %	72
	Total:	95.7 %	242

Sample S002 Clinical interpretation

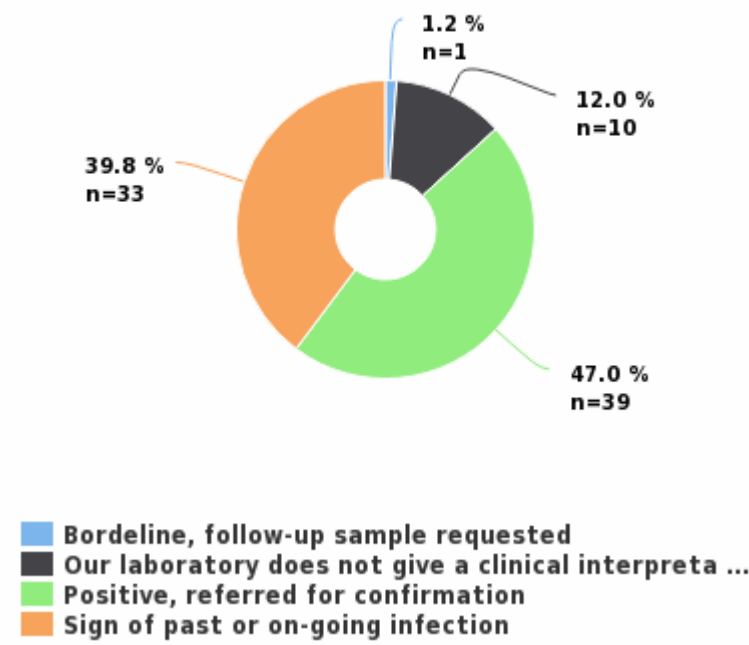


Clinical interpretation	Interpretation	Additional information	Interpretation count	Additional information count	AVR success rate	Interpretation score
	Bordeline, follow-up sample requested		1		0 %	0
	Sign of past or on-going infection		33		100 %	4
	Positive, referred for confirmation		39		100 %	4
	Our laboratory does not give a clinical interpretation to the physician		10		-	-
	Total:		83		98.6 %	


Sample S002 BorrAb



Sample S002 BorrAbG



Sample S002 BorrAbM

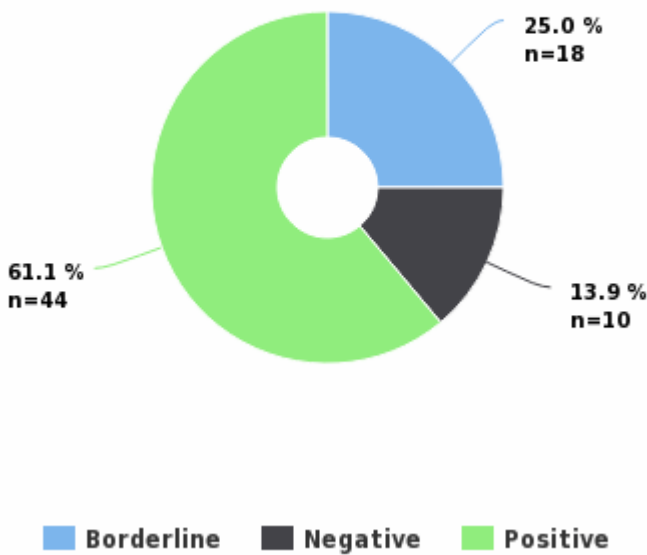

BorrAb	Interpretation	Method	Interpretation count	Method count	AVR success rate	Interpretation score
	Positive		6		100 %	2
		Immunetics C6-LYME-ELISA		6		
	Total:		6		100 %	

BorrAbG	Interpretation	Method	Interpretation count	Method count	AVR success rate	Interpretation score
	Negative		1		0 %	0
		Medac Borrelia-IgG-Elisa		1		
	Positive		80		100 %	2
		Aesku Diagn AESKULISA Borrelia IgG ELISA		1		
		Biomedica Borrelia IgG ELISA		1		
		bioMérieux VIDAS Lyme IgG		20		
		Diasorin LIAISON Borrelia IgG		28		
		Euroimmun Anti-Borrelia plus VlsE Elisa IgG		1		
		Euroimmun Anti-Borrelia Select ELISA IgG		1		
		Euroimmun Westernblot/ EUROLINE-WB IgG		2		
		In-house IFA		1		
		In-house Borrelia IgG ELISA		1		
		Mikrogen ELISA Recomwell IgG/IgM		1		
		Mikrogen Line Blot Recomblot IgG		4		
		Mikrogen recomBead Borrelia IgG		1		
		Mikrogen recomLine Borrelia IgG		2		
		Orgentec Borrelia IgG Recomb.		3		
		Siemens Enzygnost Borreliosis IgG		7		
		Thermo Scientific IDEIA Borrelia Burgdorferi IgG		1		
		Viramed Borrelia ViraStripe IgG		1		
		Vircell VirClia Borrelia IgG		1		
		Virion/Serion Borrelia burgdorferi IgG ELISA		1		
		Virotech Borrelia afzelii + VlsE IgG Europe ELISA		1		
		Virotech Borrelia Europe plus TpN17 LINE IgG		1		
	Total:		81		98.8 %	

BorrAbM	Interpretation	Method	Interpretation count	Method count	AVR success rate	Interpretation score
	Negative		10		0 %	0
		Aesku Diagn AESKULISA Borrelia IgM ELISA		1		
		Euroimmun Anti-Borrelia Select ELISA IgM		1		
		Euroimmun Lyme screen ELISA IgM		1		
		Euroimmun Westernblot/ EUROLINE-WB IgM		1		
		Mikrogen recomLine Borrelia IgM		1		
		Orgentec Borrelia IgM Recomb.		2		
		Thermo Scientific IDEIA Borrelia Burgdorferi IgM		1		
		Vircell VirClia Borrelia IgM		1		
		Virion/Serion Borrelia burgdorferi IgM ELISA		1		
	Borderline		18		100 %	2
		bioMérieux VIDAS Lyme IgM		10		

		Euroimmun Westernblot/ EUROLINE-WB IgM		1		
		Mikrogen Line Blot Recomblot IgM		3		
		Mikrogen recomBead Borrelia IgM		1		
		Mikrogen recomLine Borrelia IgM		2		
		Virotech Borrelia Europe LINE IgM Line Immunoblot		1		
	Positive		44		100 %	2
		Biomedica Borrelia IgM ELISA		1		
		bioMérieux VIDAS Lyme IgM		7		
		Diasorin LIAISON Borrelia IgM		24		
		In-house IFA		1		
		In-house Borrelia IgM ELISA		1		
		Medac Borrelia-IgM-Elisa		1		
		Siemens Enzygnost Borreliosis IgM		7		
		Viramed Borrelia ViraStripe IgM		1		
		Virotech Borrelia afzelii IgM ELISA		1		
	Total:		72		86.1 %	